

User Manual

BAYOOCARE

MyIUS-App

Release Date: 2020-07-14




Table of content

1	Symbols	4
2	Table of acronyms & definitions	5
3	Introduction	6
3.1	Legal manufacturer	6
3.2	Scope	6
3.3	Contraindications	6
4	Expected clinical benefit	7
5	Precautionary measures / safety instructions	8
6	Quick start	9
6.1	App icon	9
6.2	Splash screen	9
6.3	Menu & toolbar	10
6.4	Main navigation	11
6.5	General warnings	12
6.6	Info screens	13
6.7	Pop-ups	13
6.8	Terms of use	14
6.9	Data privacy	14
7	First time use	15
7.1	Operating system check	15
7.2	Authorization	16
7.2.1	Accepting terms of use	18
7.2.2	Accepting data privacy	18
7.3	Start setup configuration	19
7.4	Alias	20
7.5	Setup introduction	21
7.6	Introduction video	21
7.7	Baseline parameters	22
7.7.1	Age	24
7.7.2	Country	25
7.7.3	Your body	26
7.7.4	Previous contraceptive method	27
7.7.5	Pregnancy & births	28
7.8	Placement date of your IUS	29
7.9	After confirming the placement data screen	30

8 Home screen	31
8.1 Progress area	32
8.2 Weekly calendar screen	32
8.3 Monthly calendar screen	33
8.4 How to add or edit bleeding patterns	35
8.4.1 Bleeding pattern before prediction	36
8.4.2 Bleeding pattern after prediction	36
8.5 Prediction	37
8.5.1 Preconditions for a prediction	37
8.5.2 Prediction without missing days	38
8.5.3 Prediction with missing days	39
8.5.4 Prediction not allowed	40
8.5.5 Ask for a prediction	41
8.5.5.1 Step 1	41
8.5.5.2 Step 2	42
8.5.5.3 Step 3	43
9 Profile screen	44
10 Settings screen	46
10.1 How to set a notification	46
11 Notifications	47
11.1 System notifications	48
11.2 App internal notifications	48
11.2.1 Warnings about data	49
11.2.2 Warnings about app usage	49
12 Doctors report	50
13 Gems	53
14 FAQ	56
14.1 About your IUS	57
14.2 Before and after placement	57
14.3 Living with your IUS	57
14.4 How to use MyIUS	58
15 Support	59
15.1 Email	60
15.2 Hotline	60
15.3 App user manual	60
15.4 IUS user manual	60
15.5 Give feedback	61
16 Legal notice	64
16.1 Terms of use	64
16.2 Data privacy	65
16.3 Imprint	65

1 Symbols



Conform with the relevant EU guidelines.



Follow the instructions!



Medical device manufacturer

2 Table of acronyms & definitions

Abbreviation	Description
FTU	First Time Use
IUS	Intrauterine system
IFU	Instructions for use
OS	Operating System
FAQ	Frequently Asked Questions
app	MyIUS application
BMI	Body Mass Index
lb(s)	pound (symbol: lb) is a unit of mass used in the imperial and US system
kg	Kilogram is a unit of mass used in the metric system

3 Introduction

This document is the user manual that must be read prior to using the App. These instructions will also help and guide the user regarding the correct usage and understanding of the functionalities of the App.

3.1 Legal manufacturer

BAYOOCARE GmbH

Europaplatz 5

64293 Darmstadt

Tel: +49(0) 61 51 - 86 18 -0

E-Mail: info@bayoocare.com

Web: bayoocare.com

3.2 Scope

MyIUS is an application designed for persons with cycles using or planning to use Levonorgestrel Intrauterine System (LNG-IUS) contraception systems. The application is intended to accompany these users on their journey from IUS prescription over placement up to the succeeding three months and providing educational material and the option to get a prediction of future bleeding patterns. Furthermore, the application allows to record further data up to 270 days in sum.

3.3 Contraindications

MyIUS is an application designed for persons with cycles using or planning to use Levonorgestrel Intrauterine System (LNG-IUS) contraception systems. This makes the app not suitable for:

- Men
- Women not having a prescription for or not using an intrauterine system from BAYER AG
- Women suffering from Heavy Menstrual Bleeding (Menorrhagia)

4 Expected clinical benefit

As changes in bleeding profile are common to LNG-IUS users, the lack of awareness of possible bleeding changes with IUS can affect user satisfaction and further usage of this method in real world. The intended usage of the application starts with the prescription of the IUS and ends ideally after providing a most likely future bleeding profile with respect to intensity and/or regularity.

The application itself is a patient support tool or a so-called “digital companion” to be used by women using Kyleena®, Jaydess®, Mirena®. The targets of the application are the following:

- Accompanying the user from the prescription, over placement of the IUS to at least 90 days after the placement offering her useful information,
- Collecting one-time baseline parameters and continuously daily bleeding diary for at least 90 days after placement of IUS,
- Providing a prediction of bleeding profile with respect to intensity and regularity based on the collected data,
- Depending on location, collecting data beyond 90 days to improve and validate the prediction in a real-world setting
- Facilitating the communication with the HCP by providing a report comprising the daily bleeding diary and prediction.

The prediction is based on an AI model which provides the most likely future bleeding profile after the placement of the IUS. Without entering the requested information about baseline parameters and daily bleeding pattern the prediction is not available.

5 Precautionary measures / safety instructions

The app MyIUS is a clinically validated medical device and complies with the essential requirements of the 93/42/EEC directive or its national implementations.

The prediction of the bleeding pattern is only validated for the following IUS:

- Kyleena®
- Jaydess®
- Mirena®

The MyIUS app may only be used on validated smartphones and operating systems.

The current version of the app MyIUS should always be used.

The app MyIUS may not be modified without permission of the manufacturer.

The app MyIUS is not intended to be used as the sole basis for diagnosis / therapy decisions.



Note:

If you use a rooted device, the Android security mechanisms can be bypassed. Therefore, rooted smartphones are not supported for using the app, regardless of the version of the operating system.

6 Quick start

6.1 App icon

After installing the app, it shall have an application icon on the smartphone, as shown in Figure 1.



Figure 1: App icon

6.2 Splash screen

When the app is started, a splash screen containing the name of the app, the logo and the installed version of the software and the legal manufacturer info will be displayed (Figure 2).

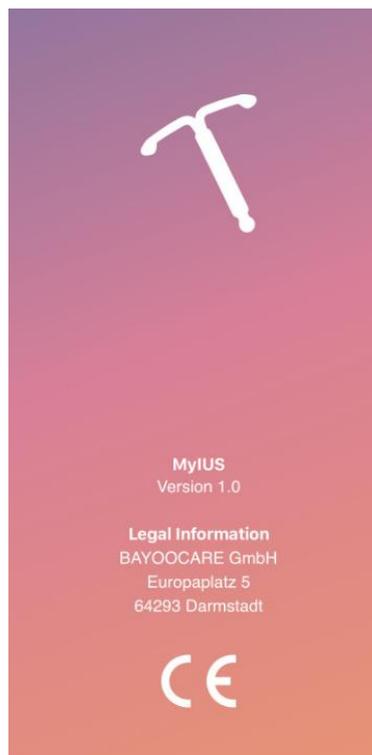


Figure 2: Splash screen at app start

6.3 Menu & toolbar

The menu  icon is displayed on the bottom right of each of the main screens.

By pressing on , seven options will be displayed and each of them navigates to one of the following sections (Figure 3):

- Profile
- Settings
- Unlocked Gems
- Prediction and doctor's report
- Frequently Asked Questions
- Support
- Legal notice

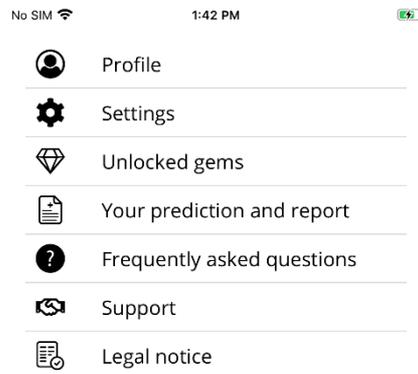


Figure 3: Burger menu

When accessing one of the sections from the Main Menu, the toolbar is also visible and contains four buttons: Home screen, unlocked Gems screen, Calendar screen and Menu icon.

6.4 Main navigation

You can navigate only from one screen further to the next one. The app does not allow you to come back to the previous screen, except for the screens belonging to the Baseline parameters. All these screens have a white arrow button on the left, as displayed in Figure 4.



Figure 4: Back icon

By pressing on the back button from a Baseline parameter screen (except Age screen), you can go back to the previous parameter screen.

6.5 General warnings

Warning pop-ups, such as the one displayed in Figure 5 will inform you about any issues with the App or with your data.

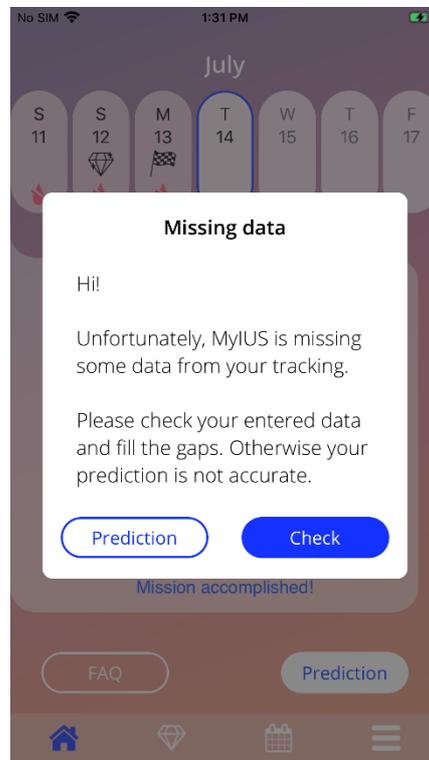


Figure 5: Warning message

Warnings will appear in the following cases:

- Upload and store of app data
- Missing baseline entries
- Missing bleeding data.
- When the app is started, and the operating system of your mobile phone is not supported.

The warning pop-ups have the following content:

- a title
- a message describing the problem that occurred
- one or two buttons representing the actions that can be realized further

6.6 Info screens

The Progress Area on the Home Screen and all the screens of Baseline parameters have a white information icon as displayed in Figure 6.

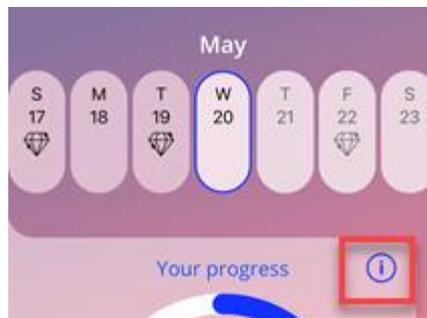


Figure 6: Information icon

When pressing on the information icon, a new pop-up will be displayed, containing detailed information about the selected section.

You can close this screen by pressing again on the information icon.

6.7 Pop-ups

Pop-up, as the one displayed in Figure 7, will appear in the following cases:

- When a reminder or notification is triggered
- When a gem is unlocked or received
- When motivational messages are provided
- When placement date is “today” or in the past and needs confirmation
- When you can confirm your placement date
- When you receive motivational messages
- When you access informational screens
- When you give feedback about the app
- When the terms of used are accessed
- When the privacy statement is accessed
- When consents for further usage are needed

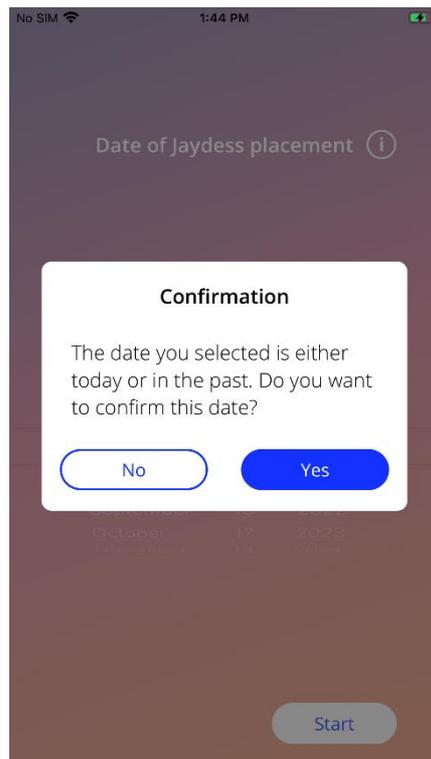


Figure 7: Pop-up message

6.8 Terms of use

The Terms of Use can be read and downloaded as PDF file, by pressing on the blue link “Terms of Use” on the Authorization screen (Figure 10). The Terms of Use will be provided according to the region and the language set on the smartphone. If the language is not supported, an English version of the Terms of Use will be displayed.

6.9 Data privacy

The Data Privacy Statement can be read and download as PDF file, by pressing on the blue link “Data Privacy Statement” on the Authorization screen (Figure 10). The Data Privacy Statement will be provided according to the region and the language set on the smartphone. If these are not supported, an English version from Great Britain of the Data Privacy Statement will be displayed.

7 First time use

7.1 Operating system check

Every time the app is launched, the operating system of your mobile is checked. In case the operation system of your mobile phone is not supported by the app version, a pop-up like the following will inform you about it.

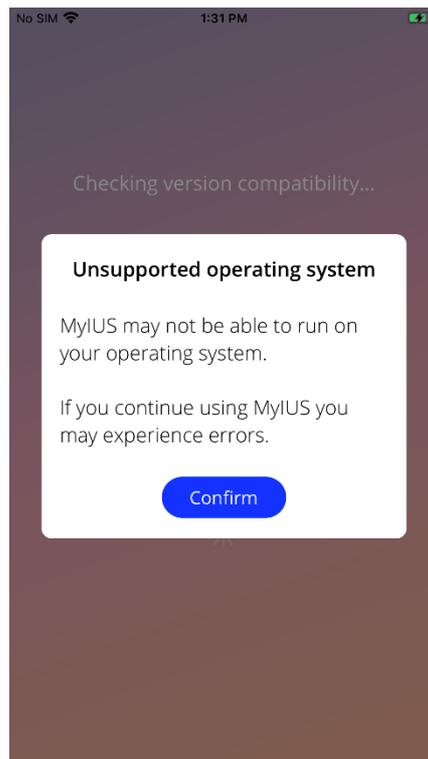


Figure 8: Pop-up message

In case the OS is not supported because it is too new, the app can be further used after giving your consent on your own risk.



Note:

If this is the case, certain functionalities might not react in the expected behavior.

In case the OS is not supported because it is too old, the app cannot be used at all.

7.2 Authorization

Once the installation has been completed and the app is launched, the “First-Time-Use” (FTU) wizard starts.

The initial screen of the FTU is the Authorization screen (Figure 10).

The authorization is mandatory. Before starting to use the app, you must follow these steps:

1. enter the authorization code consisting of four digits received from your doctor
2. read and accept the Terms of Use and the Data Privacy Statement
3. press on the “Unlock” button.



Note:

In case the Terms of Use or Data Privacy Statement is not accepted by switching on the proper toggle, the Unlock button remains disabled.



Advice:

Please read the Terms of Use and the Data Privacy Statement before accepting them.

If authorization is successful, then this screen will not be displayed anymore next time when you start the app and the app will be considered “unlocked”.

In case of a failure, a pop-up message will appear telling you that the introduced code is not correct (Figure 9).

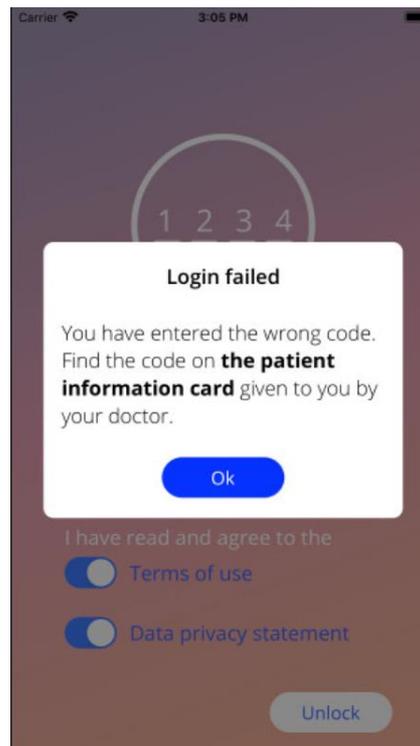


Figure 9: Login failed



Note:

In order to use the app further, you will have to enter the correct code.

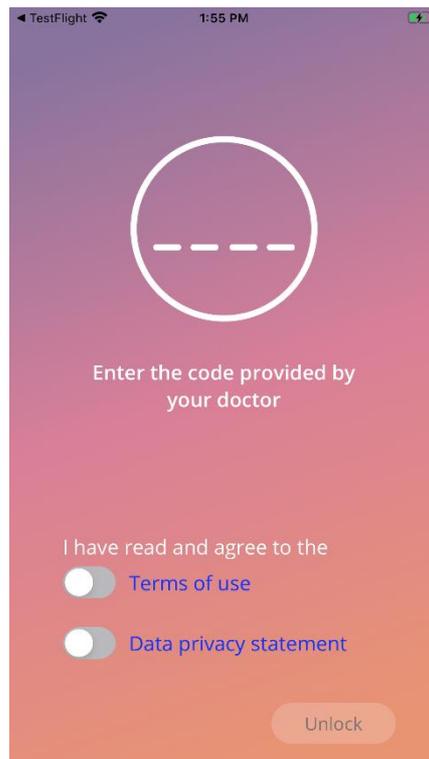


Figure 10: Authorization screen

7.2.1 Accepting terms of use

In order to proceed to the next screen, the Terms of Use must be read and accepted by pressing on the first toggle from Figure 10. Additionally, the Terms of Use can be downloaded and can be read as PDF file, by pressing on the blue link “Terms of Use”.

7.2.2 Accepting data privacy

In order to proceed to the next screen, the Data Privacy Statement must be read and accepted by pressing on the second toggle from Figure 10. Additionally, the Data Privacy Statement can be read and can be downloaded as PDF file, by pressing on the blue link “Data Privacy Statement”.

7.3 Start setup configuration

After successful authorization, the First Time Use wizard provides information about the IUS and the usage of the app. It starts with the Setup screen (Figure 11).

On this screen, the First Time Use setup can be skipped by pressing on “Skip” button from the bottom left part of the screen. In this case the Start Setup screen will be displayed again at the next app launch unless you will get to the Home Screen. You can complete your data later by accessing the Profile section.

The button “Start” from Figure 11 opens the Alias screen (Figure 12).

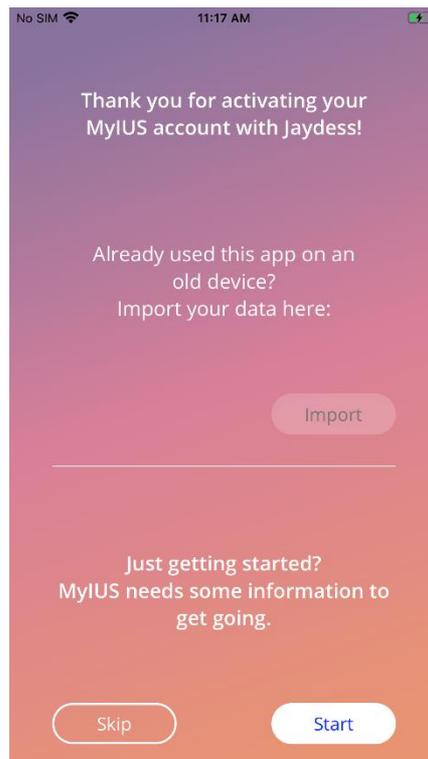


Figure 11: Start setup screen

7.4 Alias

The Alias screen (Figure 12) allows you to enter a username of maximum 15 characters. If the desired username has more than 15 characters, will be truncated to the first 15.

If the textbox for the username is left empty or you would like to change the previously set one, it can be changed later from the Profile section. The “Continue” button is enabled in this case and you can also skip this screen.

The button “Continue” opens the Introduction screen (Figure 13).

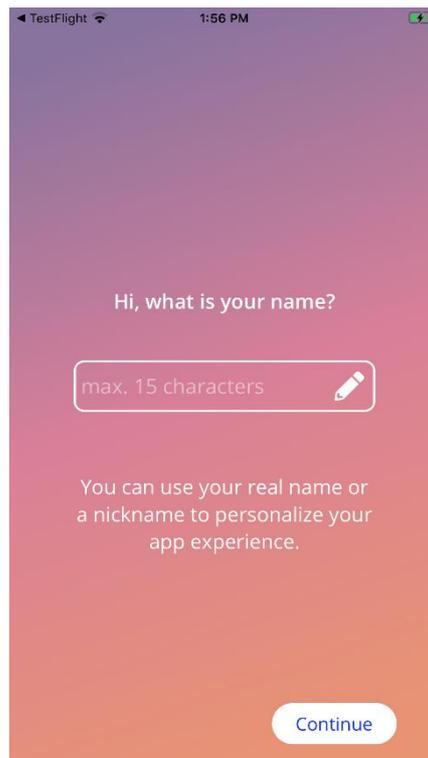


Figure 12: Alias screen

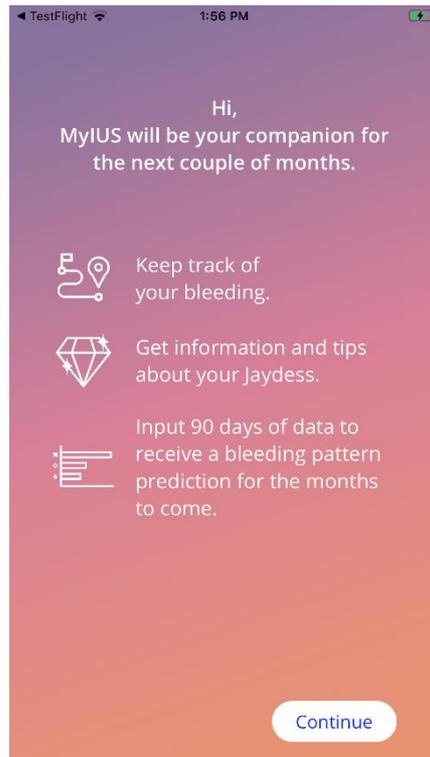


Figure 13: Introduction screen

7.5 Setup introduction

The next screen provides a short introduction text to the app usage.

The “Continue” button opens the Video screen (Figure 14).

7.6 Introduction video

This screen provides a short full screen video introducing the app usage. The video can be paused and quickly forwarded or rewinded.

The white arrow in the upper right corner of the screen opens the Start Baseline screen (Figure 15).

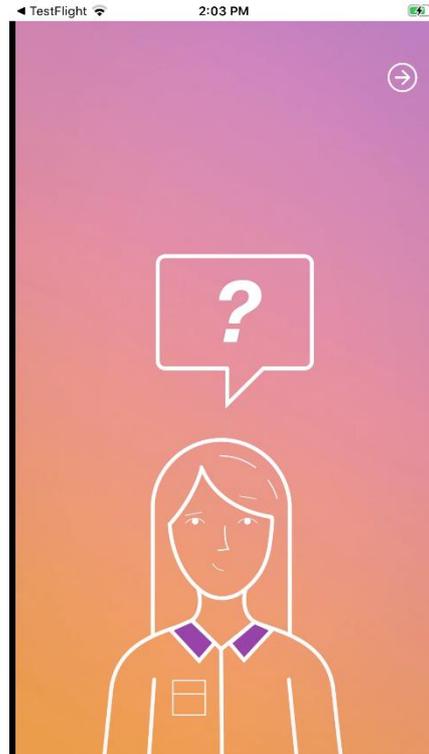


Figure 14: Video screen

7.7 Baseline parameters

In order to get an accurate prediction of your future bleeding, the app needs some information about you (Baseline parameters). Further is a questionnaire consisting of 5 steps and starts with the Start Baseline screen (Figure 15).

The Baseline questionnaire can be also skipped by pressing the “Skip” button. When pressing on “Skip”, you will be forwarded to placement date screen.

The user can start the questionnaire also from the Profile section of the Main Menu. Also from the Profile screen you will have the possibility to change the values that you set for this parameters. Each screen related to the baseline parameters gives you the possibility to return to the previous screen of the questionnaire.

Only after completing the questionnaire, you will be rewarded with a gem, as mentioned on this screen. The gem received for completing the baseline parameters needed for your future prediction is visible in the unlocked gems section. You will be able to display this gem also when you complete your baseline parameters at a later point in time from the Profile section.

All the screens belonging to the questionnaire will have the “step number” as a progress displayed on top of the screen.

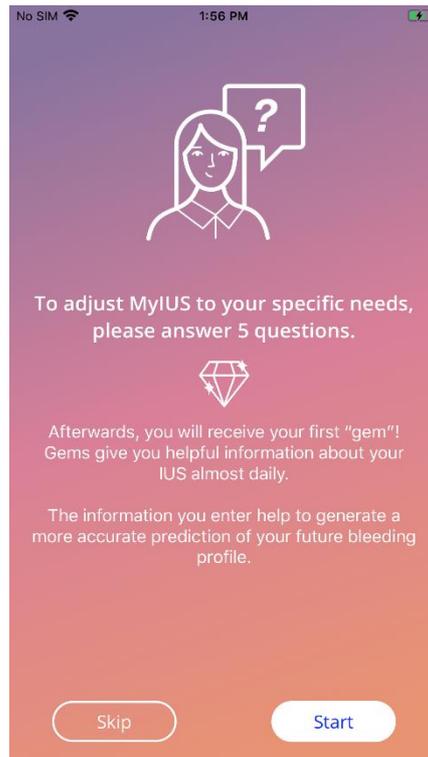


Figure 15: Start baseline screen

7.7.1 Age

This is the first screen of the questionnaire. You are asked to enter your own age in years. The ages supported are between 16 and 90 years. By default, during the FTU, there is no value selected.

You can get detailed information about how the age parameter affects the prediction of your future bleeding by pressing on the information icon.

In order to enable the “Continue” button and to proceed to the next screen you will have to select a value from the picker.

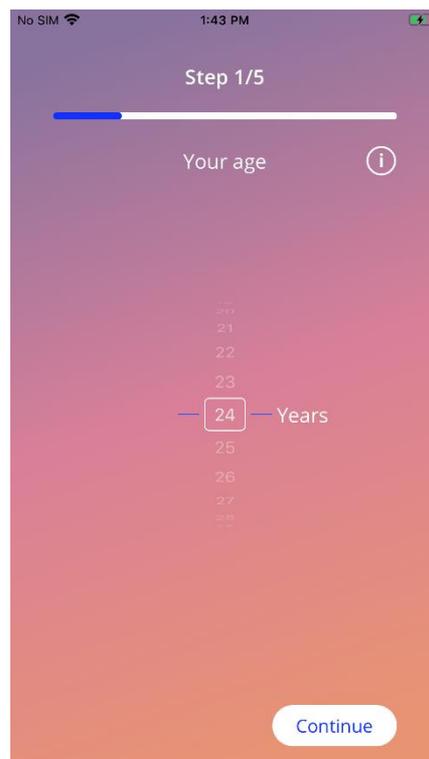


Figure 16: Age screen

7.7.2 Country

In order to predict future bleeding, the app needs also to know your country. In case the region set on your mobile phone is between the supported ones, the country will appear as preselected.

You can get detailed information about how the country parameter affects the prediction of your future bleeding, pressing on the information icon.

By pressing on the back button (white arrow), you can go back on the Age screen.

In order to enable the “Continue” button and to proceed to the next screen you will have to select a value from the picker.

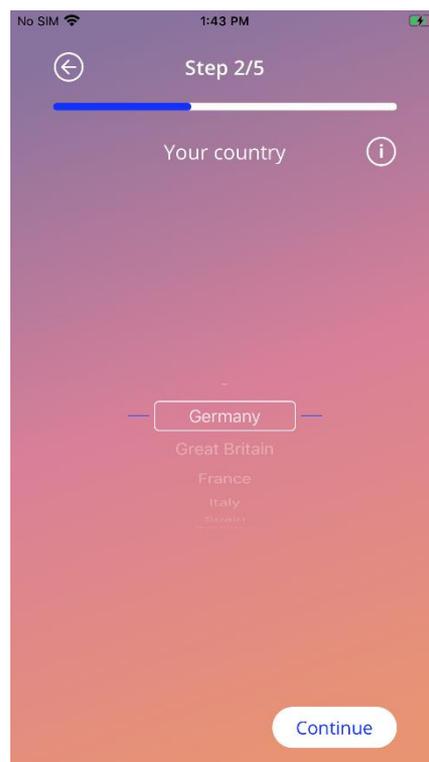


Figure 17: Country screen

7.7.3 Your body

In this screen you are asked to enter your weight, in kg or lbs. and your height in cm or ft. In order to enable the “Continue” button and to proceed to the next screen you will have to select the value from the two pickers. By default, there is no value preselected.

You can get detailed information about how the body size parameters affect the prediction of your future bleeding, pressing on the information icon. By pressing on the back button, you can go back to the Country screen.

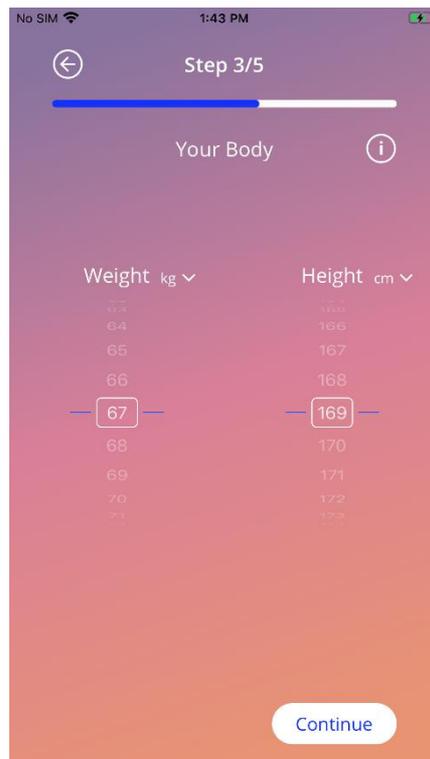


Figure 18: Body screen

7.7.4 Previous contraceptive method

The app needs also to know which contraceptive method was previously used. At least one option should be selected in order to enable the “Continue” button and to proceed to the next screen. More than one option can be selected on this screen, except when “No method” is selected.



Note:

If you already have selected other options than “No method” and after this you select this option, the previous selected options will be automatically unselected.

“No method” option cannot be used in combination with other option.

You can get detailed information about how this parameter affects the prediction of your future bleeding, pressing on the information icon.

By pressing on the back button, you can go back on the “Your body” screen.

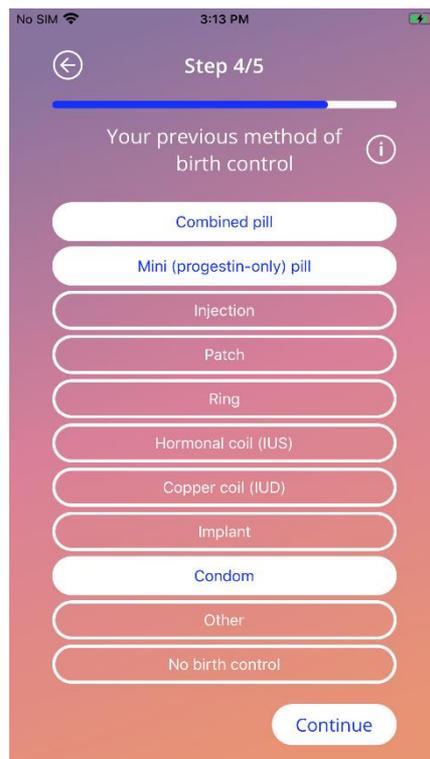


Figure 19: Contraceptive method screen

7.7.5 Pregnancy & births

The last screen of the questionnaire is about the number of pregnancies and the number of births. In order to enable “Continue” button and proceed to the next screen, values for both parameters need to be selected.



Note:

The values from the two pickers are dependent and the number of pregnancies can be only greater or equal with the number of births.

You can get detailed information about how this parameter affects the prediction of your future bleeding, pressing on the information icon.

By pressing on the back button (white arrow), you can go back on the “Previous contraceptive method” screen.

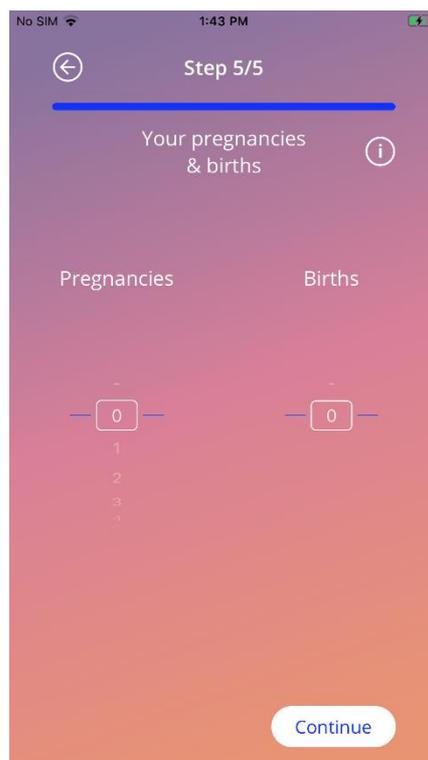


Figure 20: Pregnancy screen

7.8 Placement date of your IUS

The next screen, after the questionnaire containing the baseline parameters is the Placement date screen.

In order to get a prediction of future bleeding, the app needs to know the exact placement date of your IUS. You can set also a date in the past, up to a maximum of 90 days in the past. In this case, you will be asked in a pop-up right away to confirm the placement date or to change it by cancelling the pop-up.

By default, the “today” date will be preselected.

The placement date set can be also skipped and re-accessed or edited through the Profile section of the Main Menu.

When the placement date is reached or passed, the app asks the user at launch to confirm the placement date or, alternatively, to select another date.

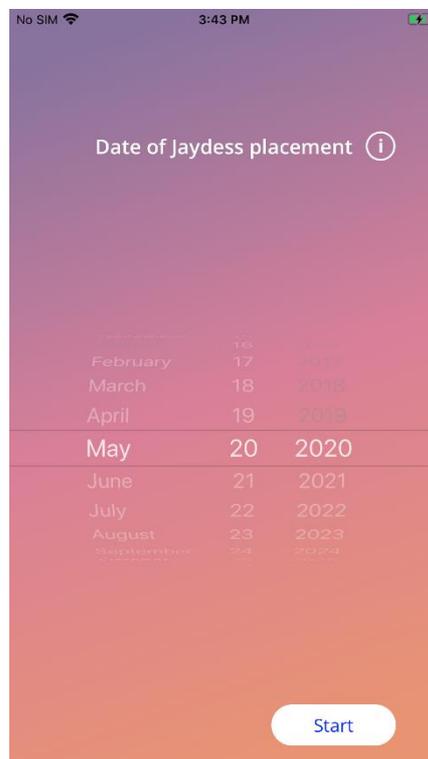


Figure 21: Placement date screen

7.9 After confirming the placement data screen

After setting a placement date and confirming it, the following screen will appear.

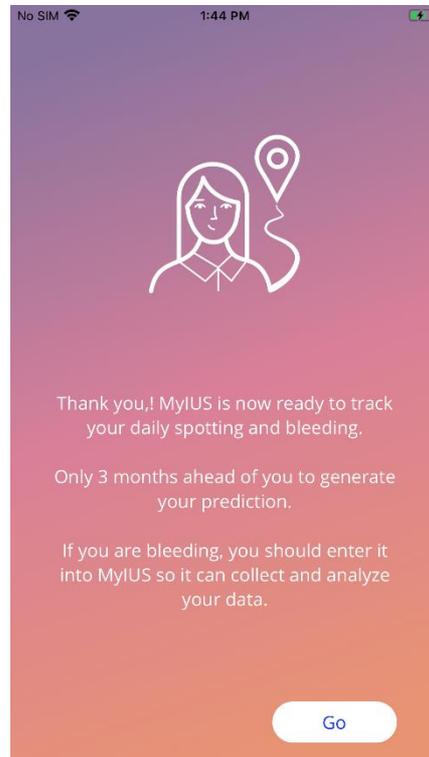


Figure 22: After confirming the placement data screen

By pressing on “Go” button, you will be forwarded to the Home Screen.

8 Home screen

The Home screen is the main screen of the app. Here you will be forwarded every time you will start the app, after configuration.

The Home screen (Figure 23) consists of three sections:

- a Weekly Calendar extract
- a Progress Area and
- a buttons area.

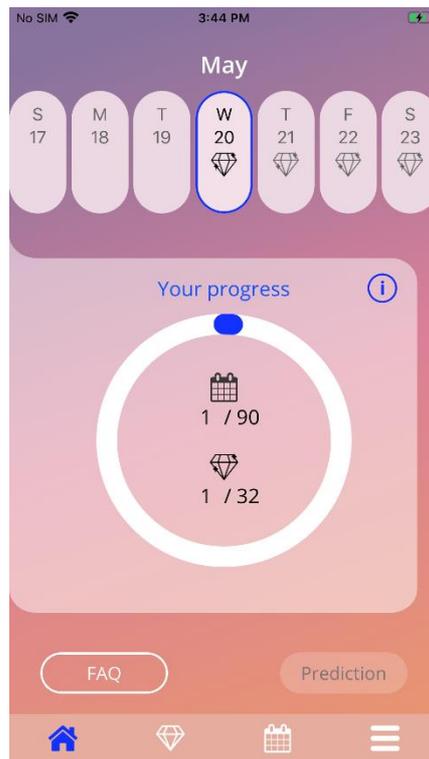


Figure 23: Home screen

8.1 Progress area

The Progress Area shows your progress related to the number of days passed since your placement date and the number of collected gems.

Every day, a new proportion of the arc of the circle will become blue, taking the day number that you are in into consideration.

Pressing on the information icon, you will get detailed information about the progress area.



Note:

This area will update only after setting and confirming your placement date of the IUS. When no placement date is set and confirmed, the number will remain 0.

In the middle of the progress area there is a read only summary representing:

- The day number that you are in after your IUS placement date from the 90 days
- The number of the unlocked gems from the total available

8.2 Weekly calendar screen

The week extract having the “today” day in the middle is displayed on the top of the Home Screen. Each day might show information related to the already introduced bleeding patterns, the prediction date and the possible gems.

Swiping to the left and right is also possible in the weekly extract with exceptions:

- When no placement date is set, the swiping functionality left and right is disabled and only the current extract is visible showing the “today” date in the middle
- When reaching the week of the placement date, swiping to the right is not possible anymore
- Swiping left dates in the future is not possible
- When one or more days are selected without having a bleeding value set

By selecting one or more days from the weekly extract will allow you to set the bleeding profile for those days.



Note:

When adding data for more than one day, you should be as accurate as possible as this may affect your future prediction.



Note:

Selection of more days is possible only in the current visible weekly extract. Swiping to weeks in the past and keeping the days selected is not possible.

The days in the future are not selectable and are also greyed out.

The gem icon display means that there is possible to receive one gem. Please see the conditions of receiving a gem in chapter 13 Gems.

8.3 Monthly calendar screen

The Monthly calendar screen (Figure 24) shows by default the current month. You can access it by pressing on the “Calendar” icon on the Navigation Toolbar from the Home Screen. When pressed, the calendar opens at the current month. Each day shows information related to already introduced bleeding profile, the prediction date and the possible gems.

In this case swiping functionality is possible in the past and in the future with no limits.

By selecting one or more days from the weekly extract will allow you to set the bleeding profile for those days.



Note:

Selection of more than one day is possible only in the currently selected month. Swiping to another month and keeping the days from the previous one selected is not possible.

The days in the future are not selectable and are also greyed out.

The gem icon display means that there is possible to receive one gem. Please see the conditions of receiving a gem in chapter 9 Gems.



Figure 24: Monthly calendar screen

8.4 How to add or edit bleeding patterns

You can add or edit an existing bleeding pattern by pressing on one or more days at the same time on the weekly calendar or on the monthly calendar. When you select more days in the same time, the same selected bleeding pattern will be entered for all the selected days.

Three patterns can be selected:

- No bleeding
- Spotting
- Bleeding

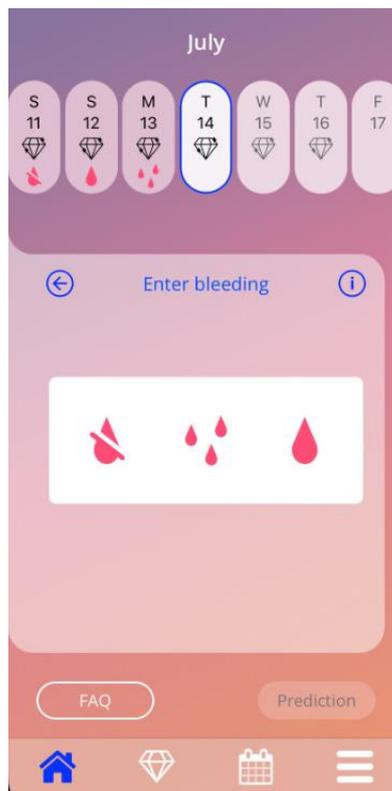


Figure 25: Bleeding pattern on home screen



Figure 26: Bleeding pattern on monthly calendar screen

8.4.1 Bleeding pattern before prediction

In case no prediction of future bleeding is still received, you can add or edit bleeding patterns only if a placement date is entered and confirmed. The selected days must be between the placement date and the current day.

8.4.2 Bleeding pattern after prediction

In case a prediction of future bleeding is received, and you have confirmed the app usage after the prediction received, it is possible to add or edit bleeding patterns between the prediction day and the current day.

8.5 Prediction

The request for a prediction for future bleeding depends on various factors, including the number of bleeding patterns entered.

8.5.1 Preconditions for a prediction

You can ask for a prediction if the following preconditions are met, in addition to the condition on the number of bleeding patterns entered:

- All the baseline parameters are set
- No previous prediction was received
- At least 90 days have passed since the placement day

When the 90th day after the confirmed placement date is reached and the bleeding pattern for this day is set, the app shall enable the “Prediction” button from the Home Screen (Figure 27).

8.5.2 Prediction without missing days

You can ask for a prediction for future bleeding if the preconditions in 4.5.1 are met and a bleeding profile is set for each day of the 90 days after the placement day.

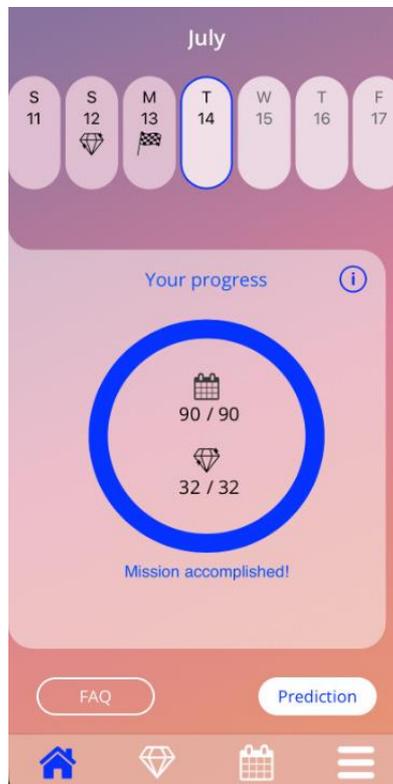


Figure 27: Prediction available screen

8.5.3 Prediction with missing days

You can ask for a prediction also if a few daily bleeding patterns are missing, provided that the pre-conditions in 4.5.1 are met and the missing patterns are at most 2 but not consecutive per 30 days period within the 90 days after a confirmed placement day.

The app shall notify you by displaying a pop-up when the previous conditions are met (Figure 28).

You can enter the missing days pressing on “Check” button and then ask again for a prediction by following the whole workflow by pressing on “Prediction” button on Home Screen (Figure 23). By pressing on “Fill gaps” button, the monthly calendar will open at the month containing the first missing bleeding data starting from the confirmed placement date.

You can also ask for a prediction without entering the missing days pressing on “Prediction” button on the pop-up.



Note:

In this case, your prediction will not be so accurate as in the case of having the whole data completed and you will not be able to change the already introduced data afterwards or add the missing data at a later point in time.

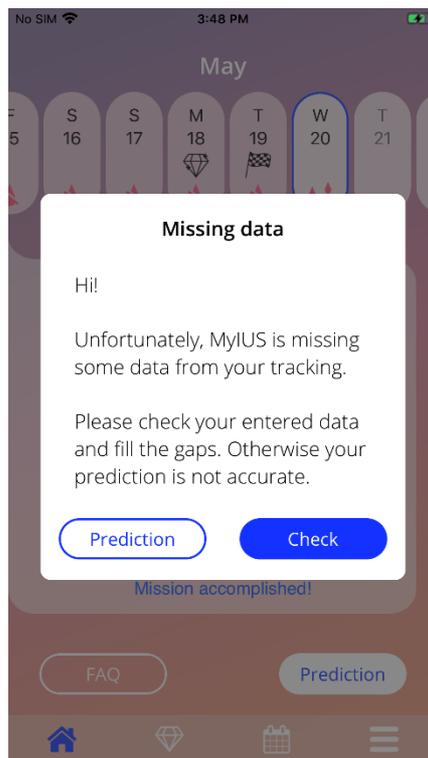


Figure 28: Missing day pop-up

8.5.4 Prediction not allowed

When at least 90 days from the confirmed placement day are passed and more than two bleeding patterns per 30 days within the 90 days after a confirmed placement day are missing, or no bleeding pattern is set for two or more consecutive days within the 90 days after a confirmed placement day, a pop-up is displayed, allowing you only to enter the missing bleeding patterns by opening the monthly calendar at the month containing the first missing bleeding data starting from the confirmed placement date.

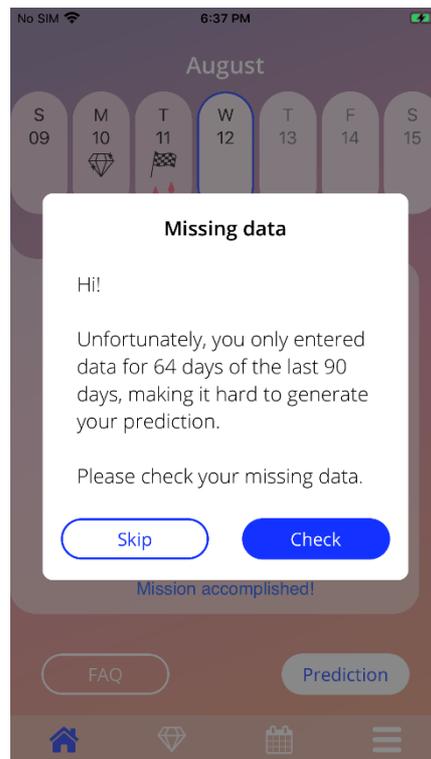


Figure 29: Too many missing data

8.5.5 Ask for a prediction

If the conditions for asking a prediction are met, you can ask for it by pressing on “Prediction” button on the Home screen (Figure 23).

8.5.5.1 Step 1

This screen tells you that you have reached the goal. You can press on “Continue” button to go to the step 2.

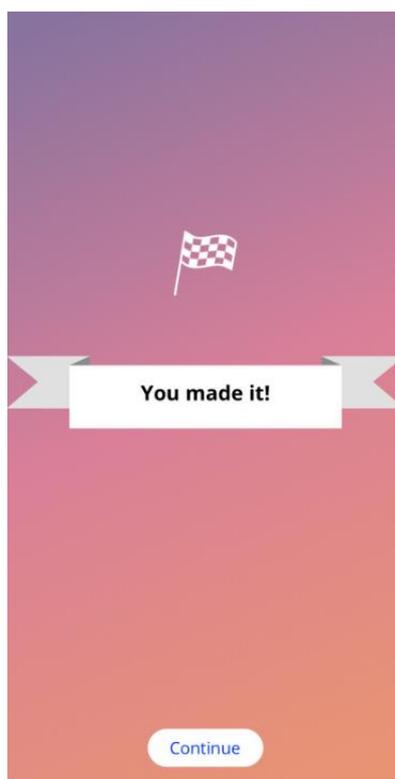


Figure 30: Prediction step 1

8.5.5.2 Step 2

This screen allows you to ask for the prediction, pressing on the “Generate your prediction” button.

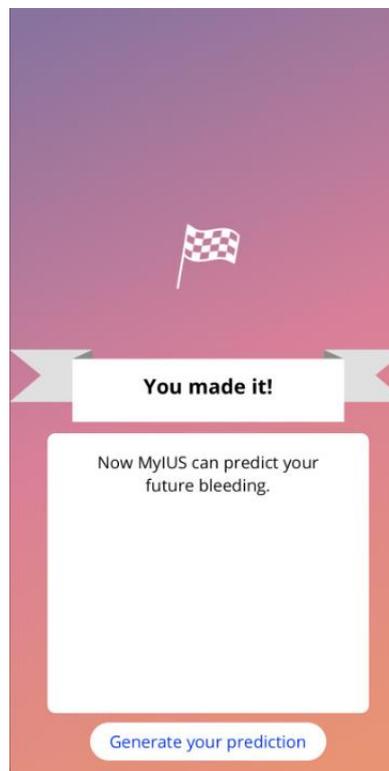


Figure 31: Prediction step 2

8.5.5.3 Step 3

This screen shows you your prediction. After that, you can go to the Home screen pressing on the “Continue” button.

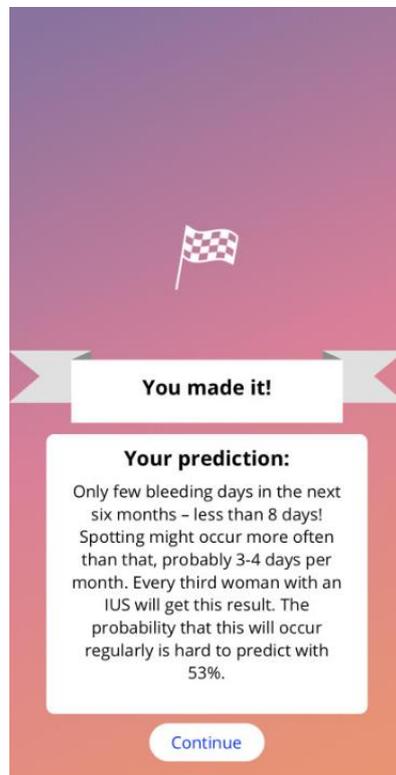


Figure 32: Prediction step 3

After receiving the prediction, the 90 days data used for it cannot be changed anymore.

The button “Prediction” will remain enabled and will always display the received prediction from this step.

9 Profile screen

The Profile screen (Figure 33) is accessible from the Main Menu , pressing on the item “Profile”. It contains three sections:

- Username
- The placement date
- The baseline parameters

You can set or modify your username by selecting the proper textbox, set or modify the placement date (please refer to 3.8) and set or modify the baseline parameters (pressing on the pencil icon).

When accessing the Baseline parameters, the whole questionnaire will start again with the Age screen (Figure 16). In case the data was already completed, it will be preselected and the “Continue” buttons will be enabled on all the screens.



Note:

You will have to go through all the screens from the questionnaire again in order to access the Profile screen again.

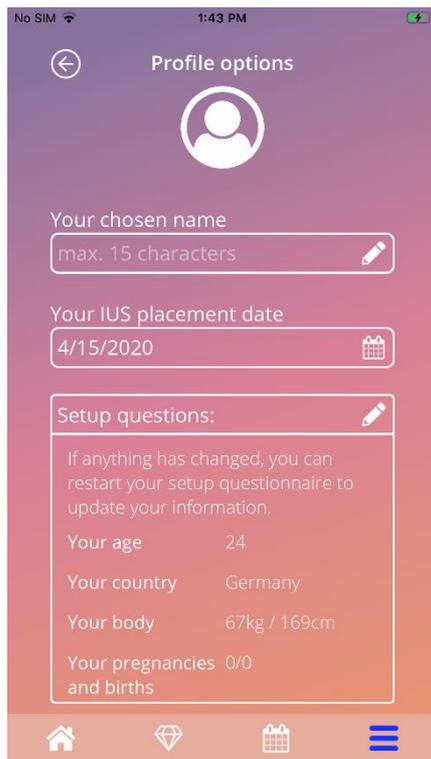


Figure 33: Profile screen

10 Settings screen

The Settings screen (Figure 34) is accessible from the Main Menu , by pressings on the item “Settings”.

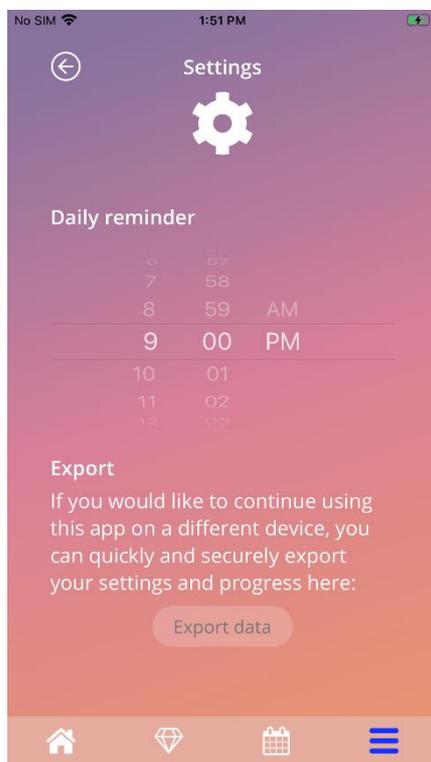


Figure 34: Settings screen

It allows you to set the time for daily reminder related to introducing the bleeding patterns and to export your data in order to import it in another app from another mobile phone.

10.1 How to set a notification

You can change the default reminder for the daily bleeding pattern (set by default to 9:00 PM), acting on the time picker on the screen. This reminder cannot be disabled, and the notification will appear on your mobile phone every day starting from the confirming of placement date until the prediction day at the set hour on this screen.

11 Notifications

Notifications can be reminders or warnings displayed by the app via pop-ups. The general appearance of a notification consists of a pop-up having:

- A title
- A text
- A button to close the pop-up

The app can display system notifications and internal notifications.

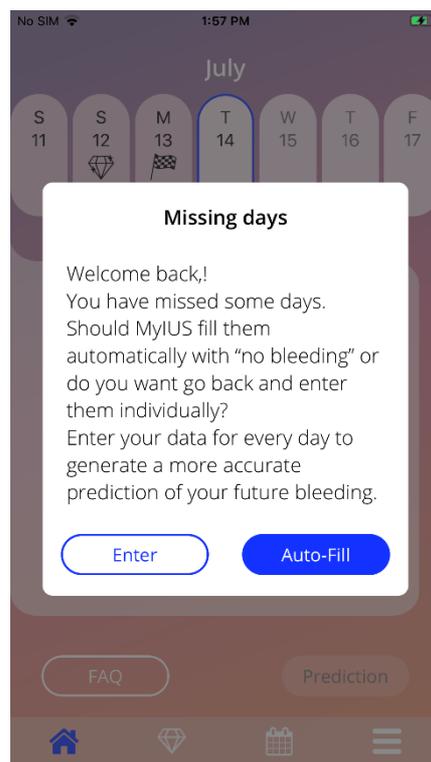


Figure 35: Reminder pop-up

11.1 System notifications

System notifications are reminders for:

- Follow-up appointment – triggers after 30 days from the confirmed placement day at 8 PM
- Planned IUS placement – triggers 1 day before planned placement day at 8.30 PM
- Daily bleeding pattern – triggers daily after confirmed placement day at 9 PM



Note:

You may not be able to see system notifications. This can have different causes, depending on your operating system.

If you are using an Android smartphone, notifications may not be displayed after a restart. To activate the notifications again, you have to create an entry in the app. The notifications will then be displayed as before.

If you are using an iOS smartphone, you must allow the app to display notifications in your device settings. Unless you allow it, you will not see system notifications outside the app.

11.2 App internal notifications

App internal notifications are mainly related to warnings about missing data or app usage. These warnings will be displayed when the app is started or comes to the foreground. You will always have the possibility to add your missing data or to close the notification.



Note:

Missing data can always lead to inconsistencies and your prediction might in the end not be so accurate as you expect.

11.2.1 Warnings about data

These warnings inform you that you have missing information or that an action will happen that has impact on your data/prediction.

They are displayed in case of:

- missing baseline parameters entries – 10 days after placement date and 5 days before prediction day
- missing daily bleeding patterns – 10 days or more with no introduced data
- missing data on prediction day (in accepted range or not acceptable for algorithm)
- placement date reached or passed
- edit of confirmed placement date that deletes the introduced daily bleeding patterns and unlocked gems
- acceptance for further usage of the app after a prediction

11.2.2 Warnings about app usage

These pop-ups warn the user that something is wrong with the app and this can lead to not being able to use the app anymore or having to redo some actions.

They are displayed in case of:

- OS not supported (too new OS version or too old OS version)
- Authorization code incorrect
- No internet connection (when QR Code is generated, when importing data, when sending feedbacks)
- Unexpected error that affects the app and needs your interaction
- Invalid QR Code
- Export or import data error
- QR Code scan error

12 Doctors report

After you get your prediction, you can generate the Doctor’s report. Figure 36 by accessing from the Main Menu , the item “Prediction and report” a preview screen will be displayed.



Figure 36: Report screen

This screen will present you just an example of how your report would look like. Your real report will be generated only when pressing on the “Open” button.



Note:

The 2 buttons will be enabled only after receiving your prediction.

In order to see your real report, you will have to press on “Open” button from the bottom left side of the screen.

After the report is generated, the default PDF viewer of your mobile phone will display you the file.

The generated report is a PDF file, with the following content:

- your name, export date, placement date, prediction date and IUS type

Name:	Export date:	Placement date:	Prediction date:	Product:
	6/4/2020	3/4/2020	6/1/2020	Jaydess

Figure 37: Report header

- baseline parameters and BMI

Your basic entries:

Age:	26	Height:	80	Previous pregnancies:	0
Country:	Germany	BMI:	98.4	Births:	0
Weight:	63	Previous contraceptive method:	Injection, Ring.		

Figure 38: Report baseline parameters

- collection of daily bleeding patterns for the 90 days before the prediction, displayed as a table with 3 rows, each of them representing a 30 days period. Each row is splitted in day number and bleeding pattern value.

 No Bleeding
 Spotting
 Bleeding

days	1	2	3	4	5	6	7	8	9	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24	25	26	27	28	29	30
Data																														
days	31	32	33	34	35	36	37	38	39	40	41	42	43	44	45	46	47	48	49	50	51	52	53	54	55	56	57	58	59	60
Data																														
days	61	62	63	64	65	66	67	68	69	70	71	72	73	74	75	76	77	78	79	80	81	82	83	84	85	86	87	88	89	90
Data																														

Figure 39: Report everyday pattern



Note:

In case for one day there is no bleeding pattern stored, the field for the “Data” will remain empty.

- 30-day interval representation as a bar chart of each of the possible values of the introduced data for the 90 days before the prediction.

Your chart:

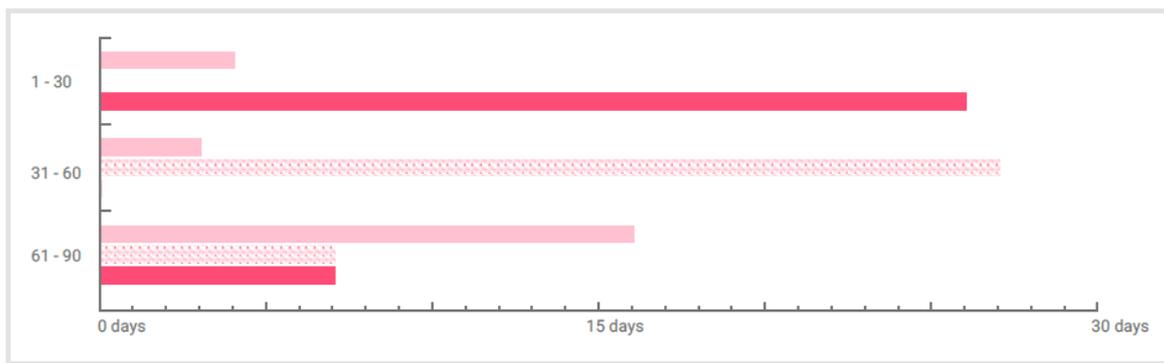


Figure 40: Report charge

- summary of 90 days bleeding patterns (how many days with no bleeding, how many days with spotting and how many days with bleeding)

Your Summary:

	No Bleeding	23/90 days
	Spotting	34/90 days
	Bleeding	33/90 days

Figure 41: Report summary

- prediction of future bleeding profile
- placeholder for comments

The report can be also downloaded as PDF file, by pressing on the “Open PDF” button.

You can also print it and send it via email, using the smartphone features by pressing on “Share PDF” button.

13 Gems

The Gems screen (Figure 42) is accessible from the Main Menu  and the toolbar by pressing on the item “Unlocked Gems”.

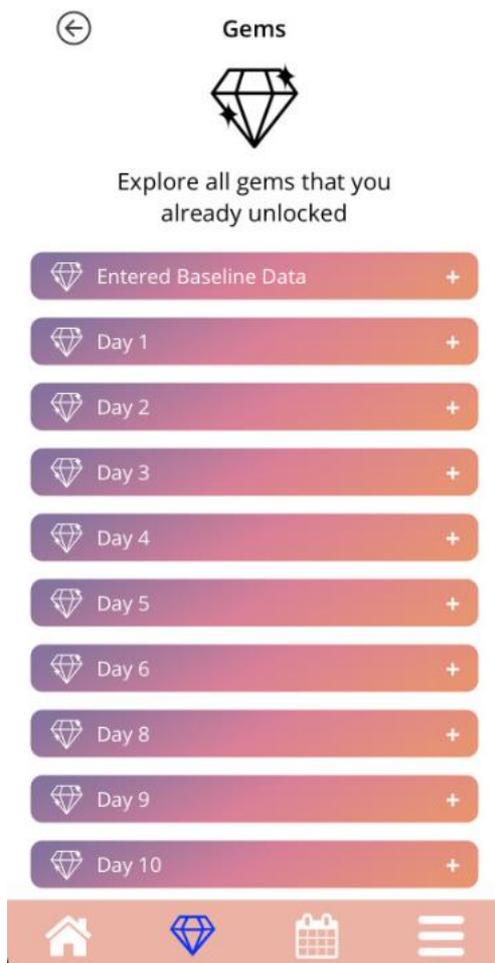


Figure 42: Gems screen

Through this screen, you can explore the “unlocked” informational gems.

An informational gem is a reward that becomes available on a fixed time basis as preconfigured in the app.

You can “unlock” an informational gem when all of the following conditions are met:

- the day with the reward is reached or passed
- at most 1 daily bleeding pattern is missing in this 30-day period until the current day
- all previous rewards of this 30-day period are unlocked
- a daily bleeding pattern for the current day is introduced

In the Gems screen you can see for each unlocked gem the day number on which it was available, and a part of the informational text related to the gem. You can display more detailed information by tapping on the “+” symbol of a day.



Note:

Not every “diamond” displayed on the monthly and weekly calendar means you have unlocked that gem. There are displayed only the days for which gems are available.

There is a special gem related to baseline parameters. This will be received automatically after completing the baseline questionnaire and will be available on top of the list in the unlocked gems section.

When you unlock one or more informational gems at once, the app will open a pop-up (Figure 43) with the following content:

- a “diamond” icon
- an informational text related to the unlocked gem or a default text
- a button for closing the pop-up
- a button to navigate to the Gems screen (Figure 42).

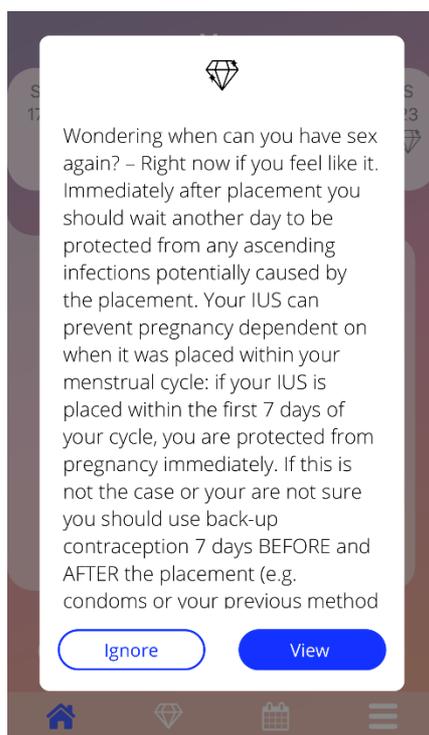


Figure 43: Informational gem pop-up

You can also receive motivational messages on a fixed time basis, depending on a constant bleeding pattern insertion. When you unlock one or more motivational gems at once, the app will open a pop-up like the one in Figure 44 having the following content:

- a motivational text related to your consistent data entering
- a button for closing the pop-up

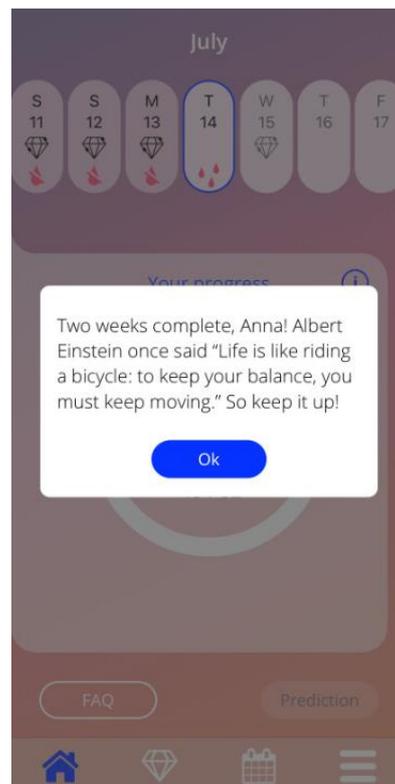


Figure 44: Motivational gem pop-up

14 FAQ

The FAQ screen (Figure 45) is accessible from the Main Menu , by pressing on the item “Frequently asked questions” or from the buttons area from the Home screen by pressing on “FAQ” button from the bottom left side of the screen.

You can access four categories:

- About your IUS
- Before and after placement
- Living with your IUS
- How to use MyIUS

You can open a category by pressing on the related button. Each category shows a list of questions about the selected topic. You can view the complete text of the answer linked to each question by pressing on the arrow button next to the question.

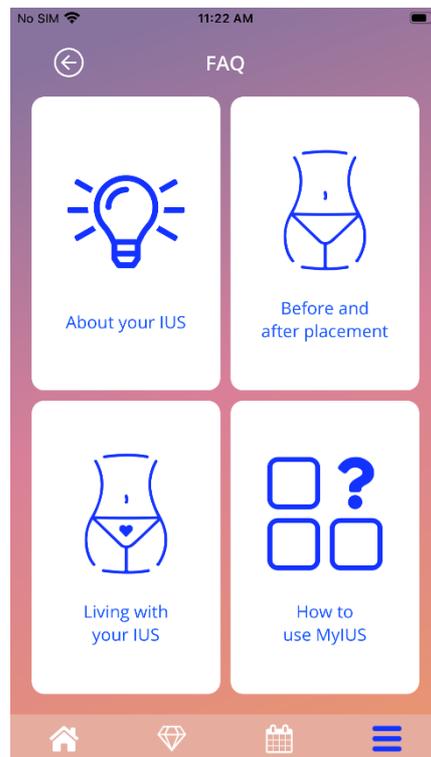


Figure 45: FAQ screen

14.1 About your IUS

This section contains general questions about the IUS, as the following:

- What is an IUS?
- How does the IUS work?
- How long does the IUS work?
- How effective is the IUS?
- Will the IUS affect my hormonal cycle?
- What are the common side effects of an IUS?
- Can certain drugs (such as antibiotics) interfere with the contraceptive effect of an IUS?
- Can the IUS affect my weight?
- Is there a risk of infection with an IUS?
- How will the IUS change my periods?

14.2 Before and after placement

This section contains questions about the placement of the IUS, as the following:

- How do I prepare for the placement of an IUS?
- How is the IUS placed?
- What can I expect right after the IUS is placed?
- Can I go swimming shortly after the IUS is placed?
- Can I use tampons or menstrual cups immediately after the IUS is placed?
- Does the IUS start working right away?
- How long should I wait to have sex after the IUS is placed?
- Is it normal to experience spotting after the IUS is placed?
- What kind of pain is normal after the IUS is placed?

14.3 Living with your IUS

This paragraph answers questions about what happens after the IUS placement, as the following:

- (How) should I check that the IUS is in place?

- Can I feel the IUS in my body?
- Can I have an MRI with an IUS in place?
- For what and how often are medical IUS assessments required?
- What if I change my mind and want to try to get pregnant?
- When do I need to replace IUS?
- Does the IUS affect my sex drive?
- Will my partner be able to feel my IUS during sex?
- Can I use a vibrator or other sex toys?
- Is it possible to displace the IUS during sex or other intense physical activity?

14.4 How to use MyIUS

This section contains general questions about the app, as the following:

- How does the prediction algorithm work? How are my predictions calculated?
- Will there be a bleeding prediction after 90 days even if I don't introduce bleeding data every day?
- What does the prediction look like and how accurate is it?
- Do I have to enter bleeding data even on days when I don't bleed or have blood spots?
- Can I change my profile name?
- Can multiple people use the app on the same device?
- Can I transfer my data to another device?
- How do I add data for past dates?
- Does the app share any of my personal data?
- How can I delete my data?
- Where can I find and manage my language settings?
- What happens after the 90 days when I received my prediction?
- How can I change the start date of my IUS use?
- How do I reset the app settings?

15 Support

The Support screen (Figure 46) is accessible from the Main Menu , by pressing on the item “Support”. This screen shows the contact information of the technical support, the App user manual and a link to your IUS user manual. You can also provide us feedback about the app, if you already received a prediction

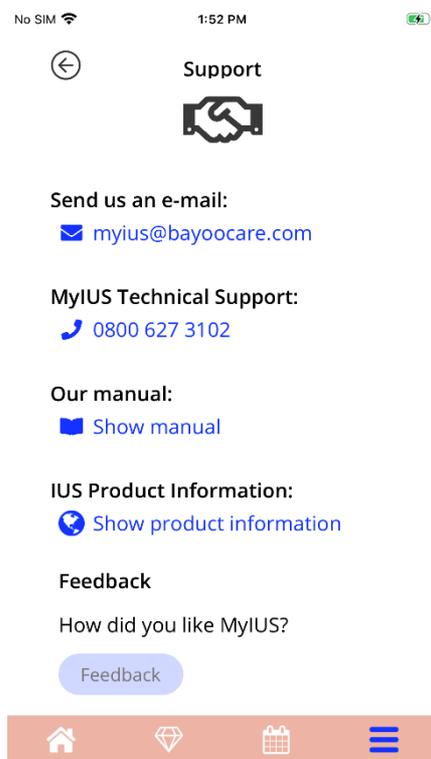


Figure 46: Support screen



Note:

No medical support will be received by using any of this contact information methods (email or phone), but technical related to the app.

15.1 Email

If you press on the given email address, the Email default app of your smartphone will open, with the recipient's address already set up.

15.2 Hotline

If you press on the given number, the phone calling feature of your smartphone will open, with the phone number already set up.

15.3 App user manual

The App user manual can be read and downloaded as PDF file, by pressing on the link "Our manual". The user manual will be provided in the language set on the smartphone, when supported.

15.4 IUS user manual

The IUS user manual can be accessed by pressing on the link. The IUS user manual will be provided in the language set on the smartphone, when supported.

15.5 Give feedback

Through the Support screen, you could send your feedback about the app, if you already received your bleeding prediction. If you press on the “Feedback” button, a pop-up asking for your consent to send your feedback to the cloud will open (Figure 47).

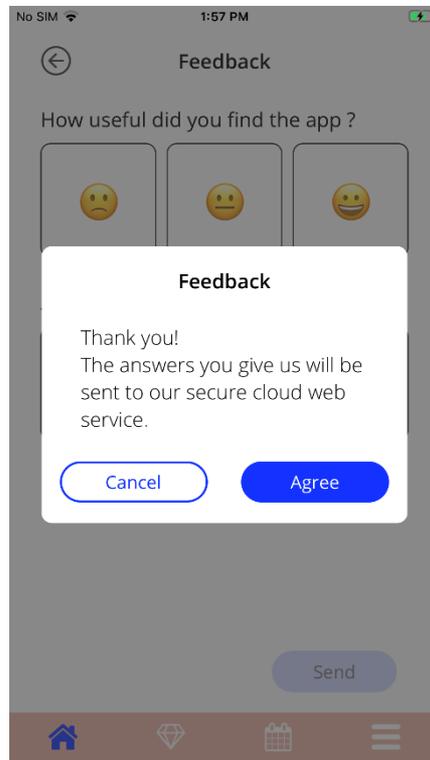


Figure 47: Feedback Consent

By pressing on the “Agree” button, the app will open the Feedback questionnaire (Figure 48). If you press on the “Cancel” button, the pop-up will close.

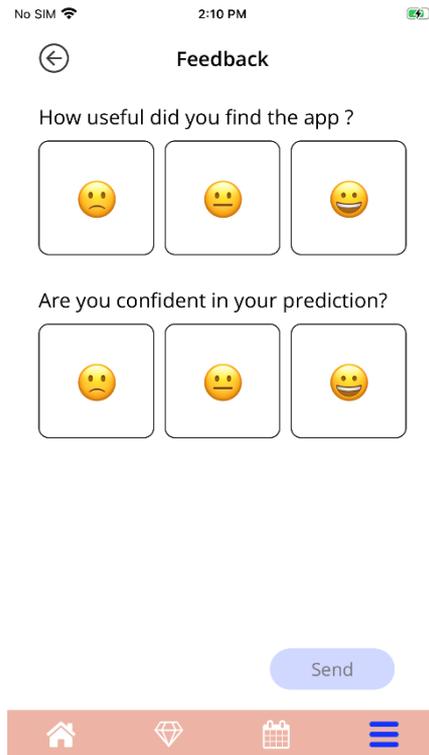


Figure 48: Feedback Questionnaire

On the Feedback questionnaire you are asked to answer 2 questions, choosing between three different answer options, displayed as a smiley icon on the pop-up.

You can also cancel the questionnaire, by pressing on the “Cancel” button. This action closes the pop-up without sending any feedback.

If you press on the “Send” button, your answer will be uploaded in the cloud. If during the upload something goes wrong, a pop-up informing you about the failure will open (Figure 49).

The app may ask you to give your feedback not only by the Support screen, but also by displaying a pop-up after you receive your bleeding prediction. If you press on the “Give feedback” button, the consent pop-up (Figure 47) will open, and you are able to open the Feedback questionnaire (Figure 47) by pressing on the “Agree” button.

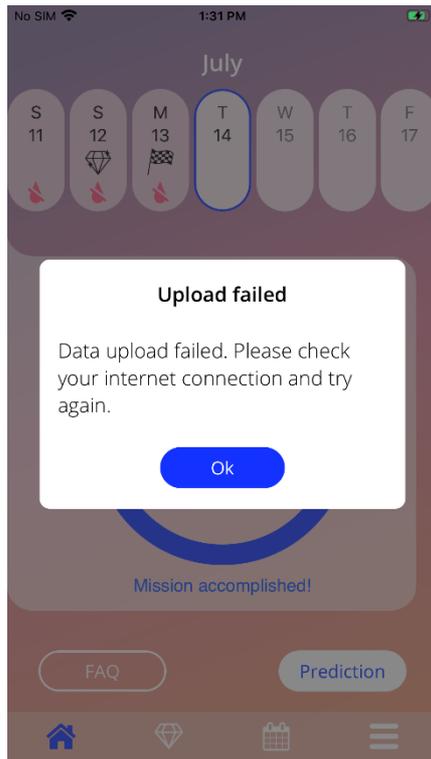


Figure 49: Upload failed pop-up

16 Legal notice

The Legal notice screen (Figure 50) is accessible from the Main Menu , by pressing on the item “Legal notice”. You can access the Terms of use, the data privacy statement and the Imprint about the manufacturer.



Figure 50: Legal notice screen

16.1 Terms of use

The Terms of Use can be read and downloaded as PDF file, by pressing on the link “Term of Use”. The Terms of Use will be provided according to the region and the language set on the smartphone. If the language is not supported, an English version of the Terms of Use will be displayed.

16.2 Data privacy

The Data Privacy Statement can be read and downloaded as PDF file, by pressing on the link “Data Privacy Statement”. The Data Privacy Statement will be provided according to the region and the language set on the smartphone. If these are not supported, an English version from Great Britain of the Data Privacy Statement will be displayed.

16.3 Imprint

The Imprint section will be further displaying and contains the following information:

- app release information
- approval numbers app texts
- approval numbers app video
- app license agreement
- MyIUS CE Marking
- License information of used libraries where applicable

Contact information about all locations of the legal manufacturer including street, city, postal code, country. The Imprint will be provided for the region set on the smartphone. If the region is not supported by the app, the Imprint valid for Great Britain will be displayed.